


Concerned that your Needleless connector could be contributing to **BSI?**

Recent publications identify only one product which has the proven track record for infection control, and has also been proven to reduce contamination of the catheter hub.^{1,2}

CLAVE[®] NeedleFree Connector

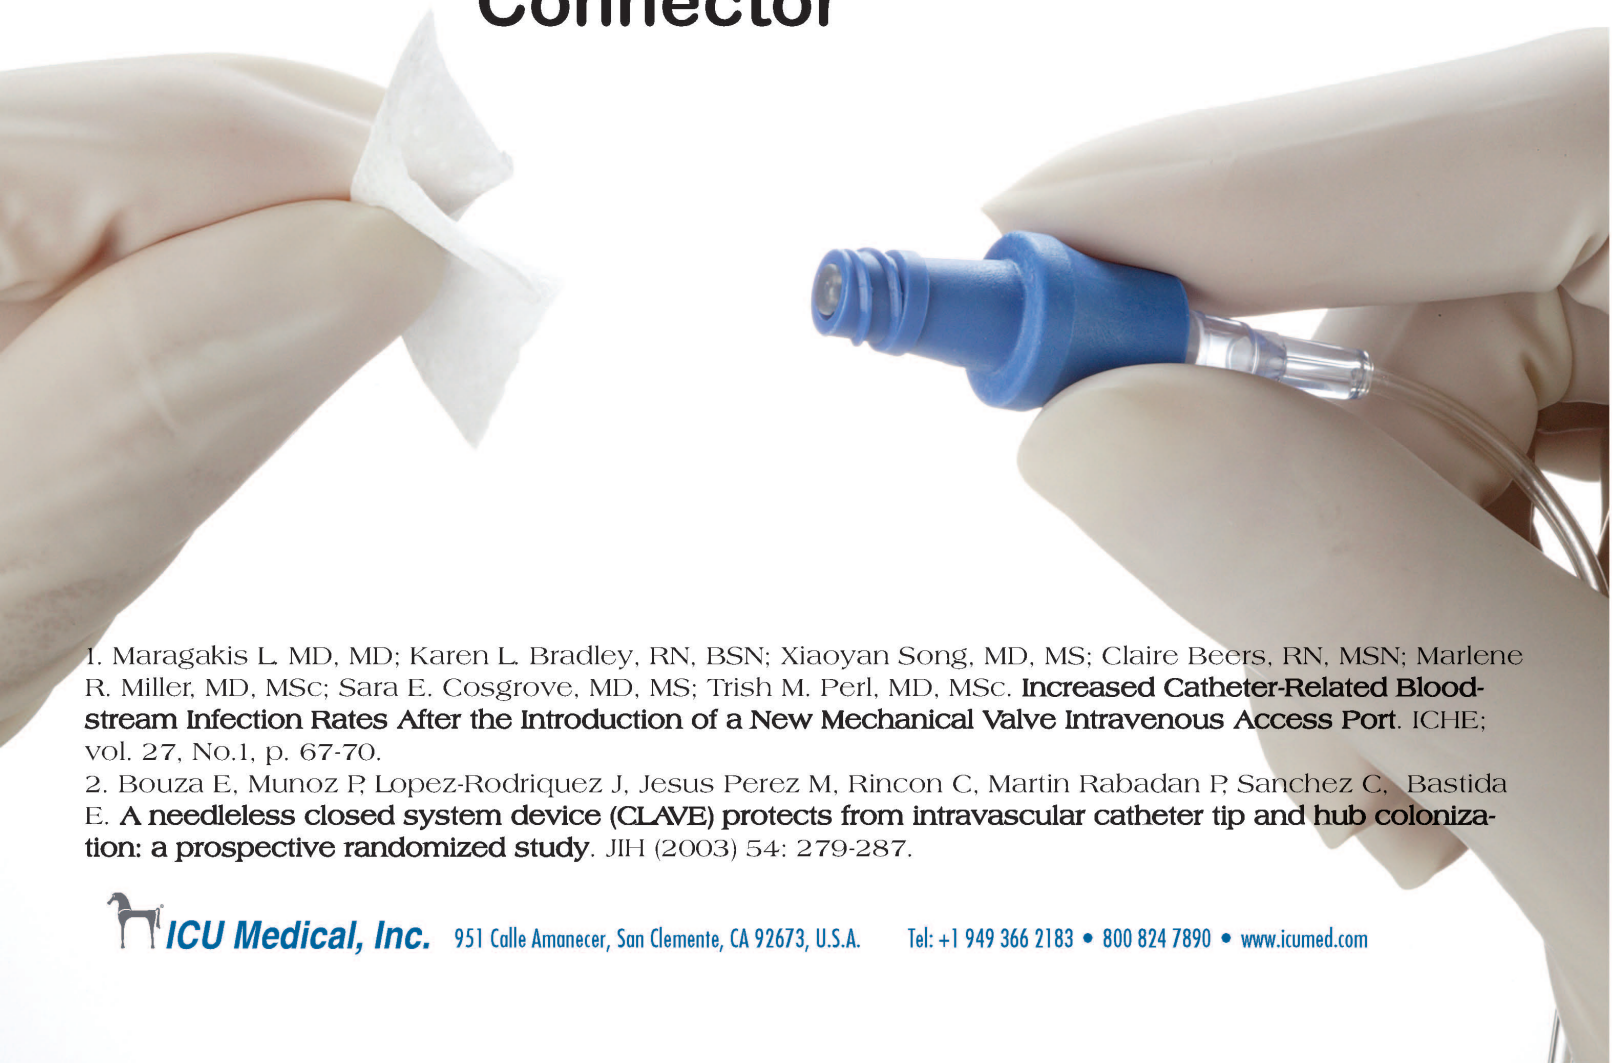

1. Maragakis L MD, MD; Karen L Bradley, RN, BSN; Xiaoyan Song, MD, MS; Claire Beers, RN, MSN; Marlene R. Miller, MD, MSc; Sara E. Cosgrove, MD, MS; Trish M. Perl, MD, MSc. **Increased Catheter-Related Blood-stream Infection Rates After the Introduction of a New Mechanical Valve Intravenous Access Port.** ICHE; vol. 27, No.1, p. 67-70.

2. Bouza E, Munoz P, Lopez-Rodriguez J, Jesus Perez M, Rincon C, Martin Rabadan P, Sanchez C, Bastida E. **A needleless closed system device (CLAVE) protects from intravascular catheter tip and hub colonization: a prospective randomized study.** JIH (2003) 54: 279-287.



ICU Medical, Inc.

951 Calle Amanecer, San Clemente, CA 92673, U.S.A.

Tel: +1 949 366 2183 • 800 824 7890 • www.icumed.com