


All Dressed Up ... Nowhere To Go.

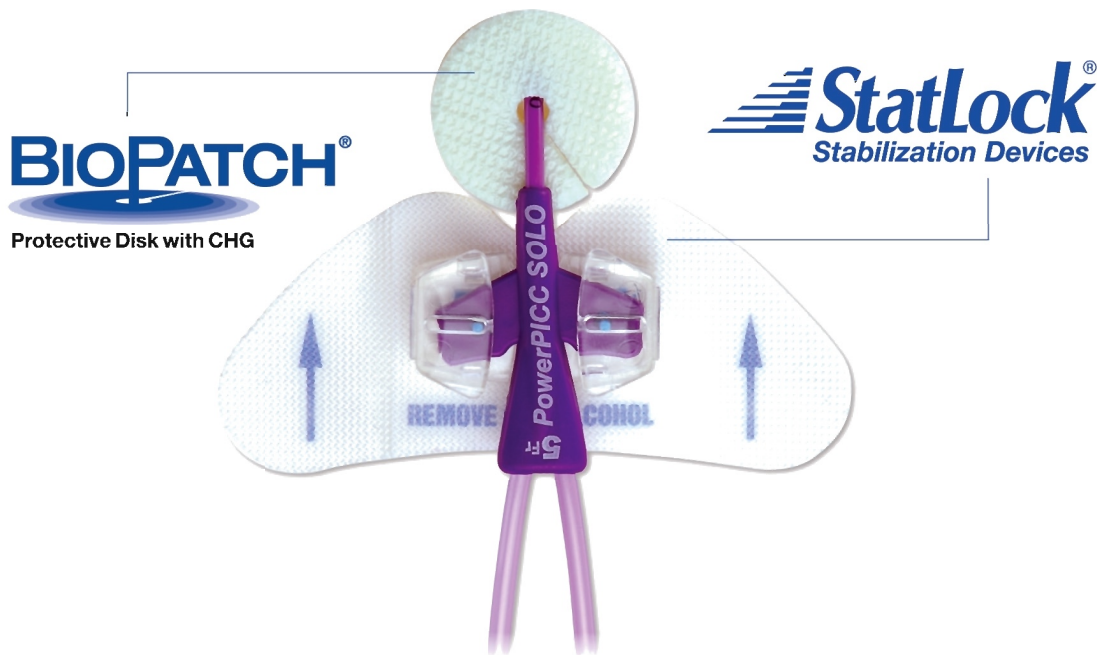

Proven To Prevent Complications

The evidence is in, and it is unparalleled. Now there is a powerful combination of clinically-proven solutions that *when partnered* together create a new standard of care by dramatically reducing the incidence of catheter-related complications.¹ Just what you would expect from Johnson & Johnson Wound Management and Bard Medical Division – both widely recognized leaders in their respective fields.

BIOPATCH® Protective Disk with CHG

It's the only one of its kind proven to reduce Catheter-Related Bloodstream Infections (CRBSI) by 60%.^{2,3} This proprietary technology continually releases CHG for up to seven days for sustained antimicrobial action.



www.BIOPATCH.com – 800.255.2500

STATLOCK® PICC Stabilization Device

This evidence-based device eliminates the need to suture central line catheters, improving patient comfort and minimizing the potential for scarring. It is also proven to reduce unscheduled restarts and increase catheter dwell times⁷, all while eliminating accidental needlesticks among healthcare workers.^{4,5,6}



www.statlock.com – 800.526.4455

1. Harnage BSN, RN, Sophie A. Achieving Zero Catheter-Related Blood Stream Infections: 15 Months Success in a Community Based Medical Center, JWA 2007 Vol 12, No 4: 218-224. 2. Maki DG, Mermel L, Genthner D, Hua S, Chiacchierini RP. An evaluation of BIOPATCH® Antimicrobial Dressing compared to routine standard of care in the prevention of catheter-related bloodstream infection, Johnson & Johnson Wound Management, a division of ETHICON, INC. 2000. Data on file. 3. When used with central venous and arterial catheters. 4. Yamamoto AJ, et al. Sutureless Securement Device Reduces Complications of Peripherally Inserted Central Venous Catheters. J Vasc Interv Radiol 2002 13:77-81. 5. OSHA Fact Sheet #7. Securing Medical Catheters. 2004. 6. Schears G, et al. Spotlight on Solutions, JCAHO/NPSF 2000. 7. Wood D, Bowe-Geddes LA. A comparative retrospective analysis of two securement techniques for peripherally inserted central catheters (PICC) and midlines in the homecare setting. JWAD 1997 Vol 2, No 3:11-16. Please refer to respective instructions for use for any indications, contraindications, hazards, warnings, cautions and directions for use. Visit www.BIOPATCH.com for Full Prescribing Information. © 2010 C. R. Bard, Inc. Bard and STATLOCK are registered trademarks of C. R. Bard, Inc. or an affiliate. BIOPATCH® is a registered trademark of Johnson & Johnson Wound Management, a division of ETHICON, INC.